

---

## Routine test

**Descr.:Freezer - Door Open Test**

23/08/2017 10:36:11

Winlog.validation 3.61

---

DIY Temperature Mapping

### General parameters

---

**Device**

Freezer

**SOP**

-

**Program**

Serial Number : 3120000444442949

**Standard**

-

**Creator**

Admin

**Charge number**

Freezer-Door Open

**Responsible**

Admin

**Validated**

23/08/2017 13:24:03

# Routine test

Descr.:Freezer - Door Open Test

23/08/2017 10:36:11

Winlog.validation 3.61

DIY Temperature Mapping

## Loggers in process

**Duration** 14400sec. **Measurement mode** Start upon start time  
**Interval** 60sec. **Start** 24/07/2017 08:00:00

# 62279772 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 12

# 62279753 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 11

# 62279751 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 10

# 62279789 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 03

# 62279782 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 07

# 62279776 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 05

# 62283272 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 01

# 62279778 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 04

# 62279773 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 06

# 62283259 Logger type: EBI 20-T Version: 1.47.0 Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 02

---

## Routine test

Descr.:Freezer - Door Open Test

23/08/2017 10:36:11

Winlog.validation 3.61

---

DIY Temperature Mapping

# 62279780      Logger type: EBI 20-T      Version: 1.47.0      Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 08

# 62283265      Logger type: EBI 20-T      Version: 1.47.0      Calibration date Refer to certificate

Channel	Type	Name
1	Temperature	Location 09

## Routine test

Descr.:Freezer - Door Open Test













23/08/2017 10:36:11

Winlog.validation 3.61

DIY Temperature Mapping



### Legend

Serial	Channel	Name
 # 62279772	1	Location 12
 # 62279753	1	Location 11
 # 62279751	1	Location 10
 # 62279789	1	Location 03
 # 62279782	1	Location 07
 # 62279776	1	Location 05
 # 62283272	1	Location 01
 # 62279778	1	Location 04
 # 62279773	1	Location 06
 # 62283259	1	Location 02
 # 62279780	1	Location 08
 # 62283265	1	Location 09


# Routine test

Descr.:Freezer - Door Open Test  
23/08/2017 10:36:11

Winlog.validation 3.61

DIY Temperature Mapping

## Total Process

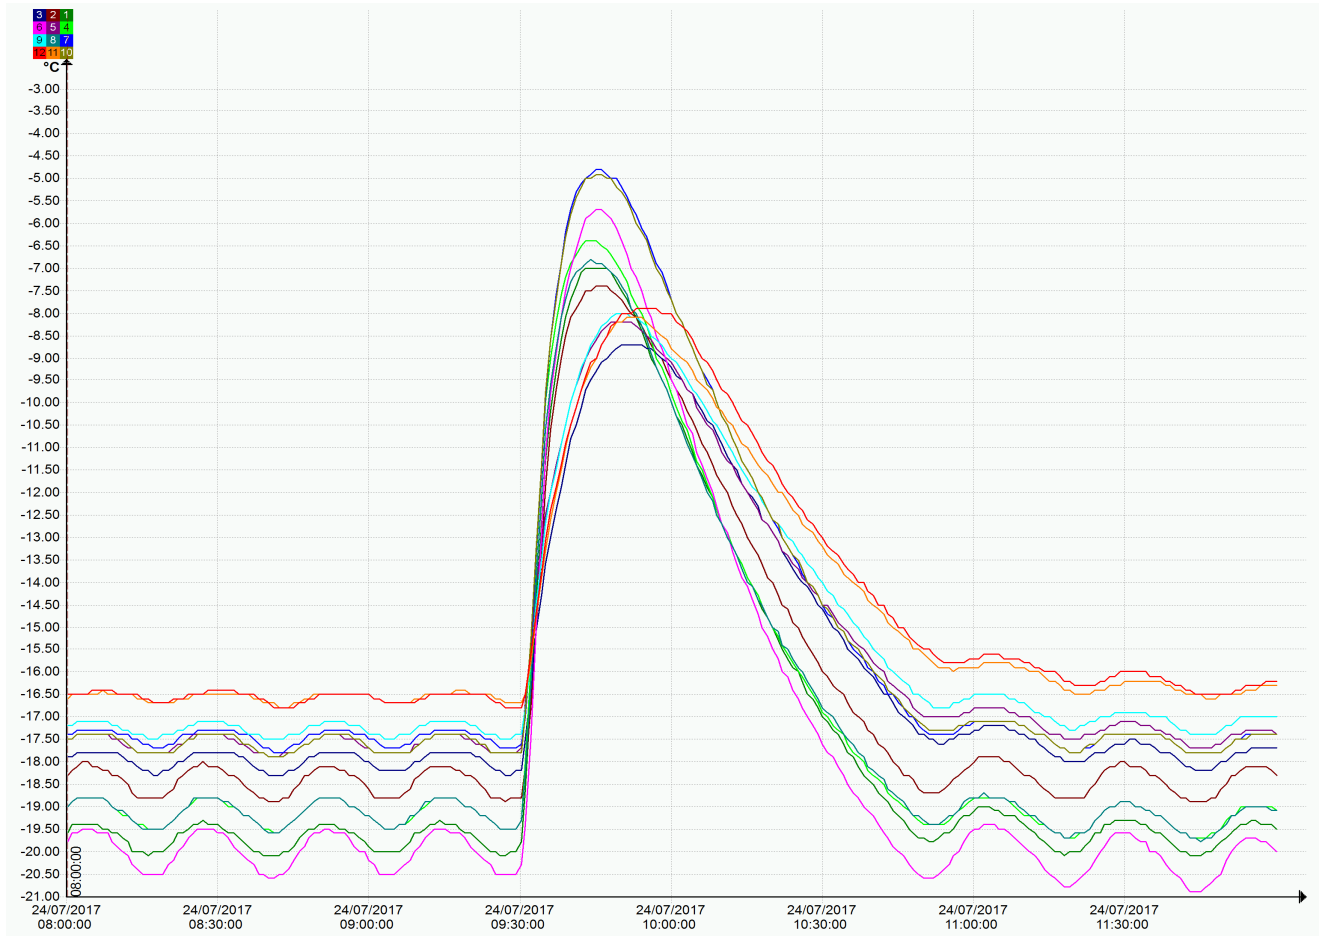

## Statistics (Total Process)

	#62279772	#62279753	#62279751	#62279789
	1	1	1	1
<b>Max</b>	-7.00 °C	-7.40 °C	-8.70 °C	-6.40 °C
<b>Mean</b>	-17.54 °C	-16.54 °C	-16.09 °C	-17.12 °C
<b>Min</b>	-20.10 °C	-18.90 °C	-18.30 °C	-19.70 °C

	#62279782	#62279776	#62283272	#62279778
	1	1	1	1
<b>Max</b>	-8.20 °C	-5.70 °C	-4.80 °C	-6.80 °C
<b>Mean</b>	-15.71 °C	-17.81 °C	-15.33 °C	-17.16 °C
<b>Min</b>	-17.90 °C	-20.90 °C	-17.80 °C	-19.80 °C

	#62279773	#62283259	#62279780	#62283265
	1	1	1	1
<b>Max</b>	-8.00 °C	-4.90 °C	-8.10 °C	-7.90 °C
<b>Mean</b>	-15.43 °C	-15.37 °C	-14.81 °C	-14.68 °C
<b>Min</b>	-17.50 °C	-17.90 °C	-16.80 °C	-16.80 °C